

Product Instruction

Fentanyl Test Strip (liquid/powder)

Ref. No: FENT24

For Forensic Use Only. Not for IVD

WARNING: THIS TEST DOES NOT EVALUATE DRUG SAFETY OR PURITY

INTENDED USE

Instanosis Fentanyl Test Strip (liquid/powder) is a rapid immunoassay visual test for the qualitative detection of fentanyl in suspicious substances at the cut-off concentration of 5 ng/ml.

COMPONENTS

- Individually packed test strips
- Product Instruction

PROCEDURE AND RESULT INTERPRETATION

- For powders, it is recommended to completely dissolve about 0.5 mg of sample in about 5 ml (1/5 oz) of water.
- For liquid samples, use directly.
- Follow the instructions on the back.



LIMITATIONS

- The product is for forensic use and should only be used for the qualitative detection of fentanyl.
- A contaminated or tainted sample may give false results.
- Technical or procedural errors may cause false results.
- Other chemicals may interfere with the test and cause false results.

- This test provides only a preliminary result. A more specific alternative method must be used to obtain a confirmed analytical result. Clinical consideration and professional judgment should be exercised with any drug of abuse test result, particularly when the preliminary test result is positive. Gas or liquid chromatography/mass spectrometry is the preferred confirmatory method.

PRECISION

Test precision was determined by blind tests with control spiked solutions. Solutions with fentanyl concentration at 50% of the cut-off (2.5 ng/ml) yielded negative results. Solutions with fentanyl concentration at 150% of the cut-off (7.5 ng/ml) yielded negative results.

SPECIFICITY

The following compounds were identified to cause false positive results at 5 minutes when tested at 10 µg/ml.

Risperidone 2-hydroxy risperidone Isoxsuprine

The following compounds were found not to cause false positive when tested at concentrations of 100 µg/ml or higher.

Acetaminophen	Acetone	Acetophenetidin	Acetylsalicylic acid	Albumin	Albuterol	Aminopyrine	Amitriptyline
Amobarbital	Amoxicillin	Ampicillin	Apomorphine	Ascorbic acid	Aspartame	Atropine	Benzilic acid
Benzoic acid	Benzoyllecgonine	Bilirubin	Boric acid,	Bupropion	Caffeine	Carbamazepine	Chloramphenicol
Chlorothiazide	Chlorpromazine	Cholesterol	Clomipramine	Clonidine	Cortisone,	Cotinine	Creatinine
Deoxycorticosterone	Desipramine	Diclofenac	Diflunisal	Digoxin	Chloral hydrate		
DL-Tryptophan	DL-Tyrosine	Doxepin	Ephedrine	Erythromycin	Ethanol	Fenpropfen	
Fluphenazine	Furosemide	Galactose	Gamma globulin,	Gentisic acid	Glucose	Hemoglobin	Hydralazine
Hydrochlorothiazide	Hydrocortisone	Hydroxytyramine	Ibuprofen	Imipramine	Isoproterenol	Meprobamate	β-Estradiol
Ketoprofen	Labetalol	Lidocaine	Loperamide	Maprotiline	Zomepirac		Methapyrilene
Uric acid	Methoxyphenamine	Metronidazole	Acceainide	NaCl	Nalidixic acid	Verapamil	Venlafaxine
Naproxen	Niacinamide	Nicotine	Nifedipine	Norethindrone	Nortriptyline	Noscapine	Octopamine
O-Hydroxyhippuric acid	Oxalic acid	Oxazepam	Oxolinic acid	Oxymetazoline	Papaverine	Penicillin G	Perphenazine
Phencyclidine	Phenetizine	Phenobarbital	Prednisone	Propoxyphene	Propranolol	Pseudoephedrine	Quinine
Ranitidine	Riboflavin	Salicylic acid	Secobarbital	Serotonin	Sulfamethazine	Sulindac	Tetrahydrocortisone
Valproic acid	Tetrahydrozoline	Thiamine	Thioridazine	Triamterene	Trifluoperazine	Trimethoprim	Tyramine

1-(3-chlorophenyl) Piperazine	6-Acetyl morphine	Amphetamine	Buprenorphine	Δ9-THC	Ceftriaxone	Ciprofloxacin	Cocaine
Codeine	Dextromethorphan	Dihydrocodeine	Diphenhydramine,	Duloxetine	EDDP	EMDP	Trazodone
Fluoxetine	Haloperidol	Heroin	Hydrocodone	Hydromorphone	Ketamine	Levorphanol	Chlorophenylpiperazine
MDMA	Meperidine	Methadone	Methamphetamine	Morphine	Morphine-3-glucuronide	Naloxone	Naltrexone
Norbuprenorphine	Norcodeine	Norketamine	Normeperidine	Normorphine	Noroxycodone	Ofloxacin	Oxycodone
Oxymorphone	Pentazocine	Pipamperone	Quinidine	Tapentadol	Thioridazine		
Tramadol	Tramadol-N-Desmethyl	Tramadol-O-Desmethyl	Urea				

SYMBOL	MEANING
	Consult instruction for use
	Batch code
	Catalog number
	Do not reuse
	Store between 36-86°F (2-30°C)
	Use by date
	Do not use if package is damaged

Manufactured By:

Instanosis Inc.

1004 w 9th Avenue, Suite 10


King of Prussia, PA 19406

www.instanosis.com

customerservice@instanosis.com



Toll Free: 1-800-946-5430

Hours of Operation: Monday – Friday 9am – 5pm (EST)

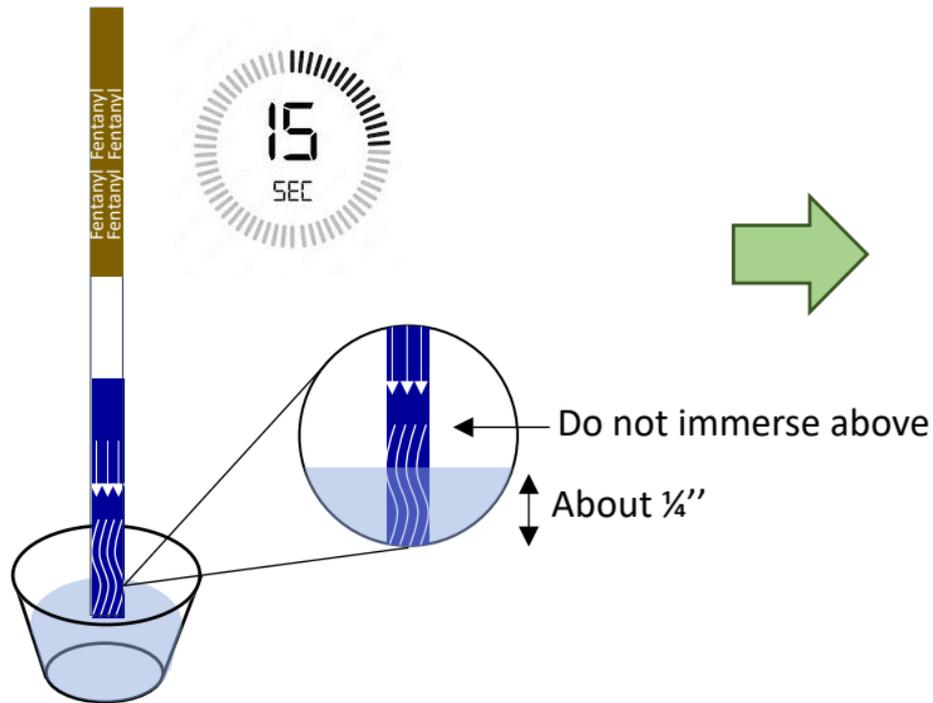


Step 1

Dip the strip in the liquid and hold for 15-20 seconds. You should see water migrating up.

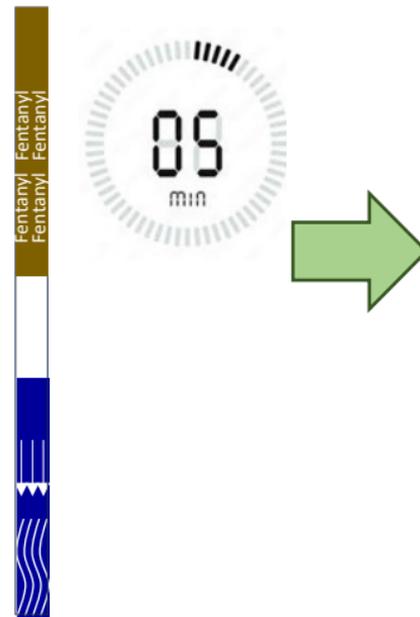

Step 2

Take the strip out and place it on a non-absorbent flat surface. Wait for 5 minutes.

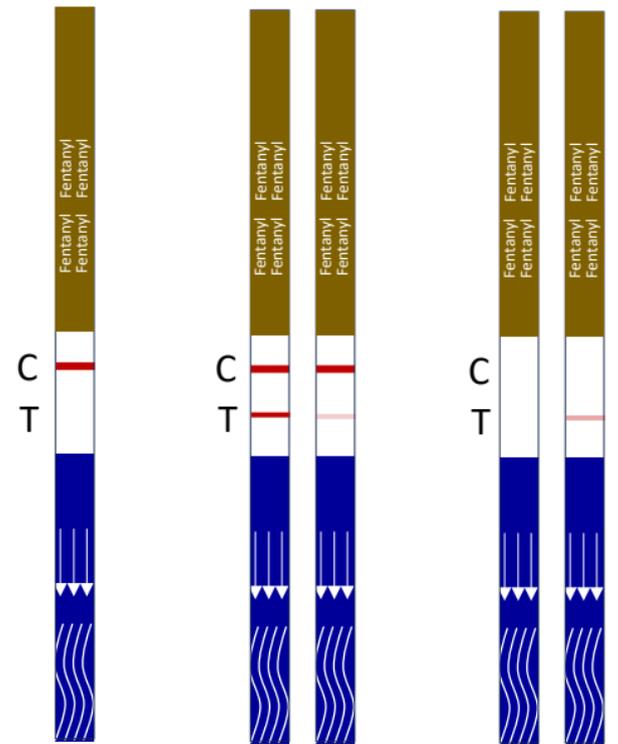

Positive

Negative

Invalid

Step 3

Compare with the pictures to read result.
Do not read after 2 hours.